



Division of Criminal Justice Services

CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 142306, performed on May 25, 2021 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under
ESRA by Joshua Vinehout
on 6/2/2021 3:03 PM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Geddes Town Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT
Date: May 25, 2021 Serial Number: 142306

Reference Solution Lot Number: 20361
Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.01 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.099 %	34.01 degrees centigrade
4	0.099 %	34.01 degrees centigrade

Reference Solution Lot Number: 20470
Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.079 %	34.01 degrees centigrade
2	0.079 %	34.01 degrees centigrade
3	0.079 %	34.01 degrees centigrade
4	0.079 %	34.01 degrees centigrade


Reference Solution Lot Number: 20290
Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.181 %	34.01 degrees centigrade
2	0.180 %	34.01 degrees centigrade
3	0.180 %	34.01 degrees centigrade
4	0.180 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 142306, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under
ESRA by Martin Schilling
on 5/25/2021 1:35 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45926

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 5/26/2021 1:42 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Geddes Town Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 142306
Date: May 25, 2021

- 1. General Appearance and condition of this device -----: **OK**

- 2. Check controls and indicators -----: **OK**

- 3. Check breath flow system -----: **OK**

- 4. Check printer operation -----: **OK**

- 5. System cycles through all modes -----: **OK**



6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION

Performed by:

Digitally signed under
ESRA by Martin Schilling
on 5/25/2021 1:35 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45926

Reviewed by:

Digitally signed under
ESRA by Frank Sgarlata
on 5/26/2021 1:42 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

GEDDES TOWN
POLICE DEPT
DATAMASTER dmt: 142306





Date: 05/25/2021

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: ~~4926~~ 45926 MJJ 5/25/21
Operator Agency/Dept: GEDDES TOWN PD
Reference Standard #: 20361

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:25
INTERNAL STANDARD	VERIFIED	12:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:25
BLANK TEST	0.000	12:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:26
BLANK TEST	0.000	12:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:27
BLANK TEST	0.000	12:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:29
BLANK TEST	0.000	12:30

Average = 0.0990
Std Dev = 0.0000

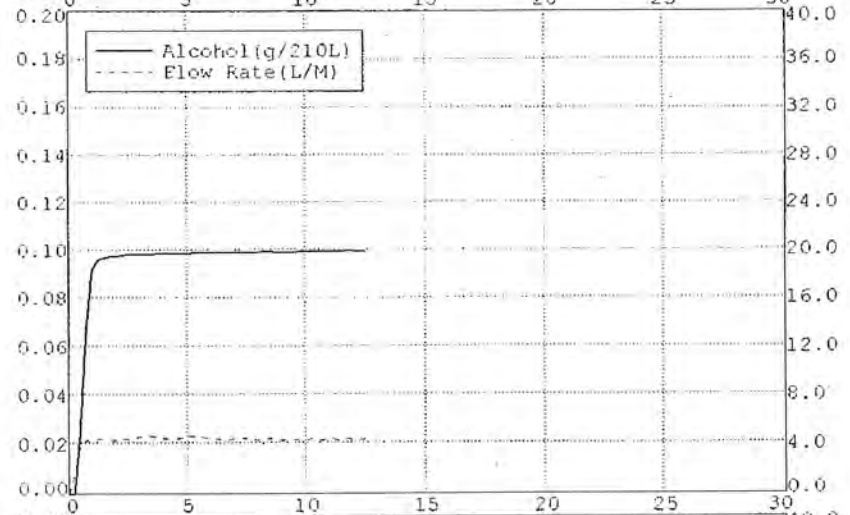

TECHNICIAN TEST

GEDDES TOWN
 POLICE DEPT
 DATAMASTER dmt: 142306


Date: 05/25/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: GEDDES TOWN PD
 Reference Standard #: 20470

Nominal = 0.080 g/210L

BLANK TEST	0.000	12:32
INTERNAL STANDARD	VERIFIED	12:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	12:32
BLANK TEST	0.000	12:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	12:34
BLANK TEST	0.000	12:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	12:35
BLANK TEST	0.000	12:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.079	12:36
BLANK TEST	0.000	12:37

Average = 0.0790
 Std Dev = 0.0000



TECHNICIAN TEST

GEDDES TOWN
 POLICE DEPT
 DATAMASTER dmt: 142306





Date: 05/25/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: GEDDES TOWN PD
 Reference Standard #: 20290

Nominal = 0.180 g/210L

BLANK TEST	0.000	12:40
INTERNAL STANDARD	VERIFIED	12:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.181	12:40
BLANK TEST	0.000	12:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:41
BLANK TEST	0.000	12:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:43
BLANK TEST	0.000	12:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:44
BLANK TEST	0.000	12:45

Average = 0.1802
 Std Dev = 0.0005



**SIMULATOR
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Geddes Town Police Department
Manufacturer: GUTH LABORATORIES Model: 12V500
Serial Number: MP4203
Date: May 25, 2021

Breath Simulator Temperature
34.02 degrees centigrade



Martin Schilling
Highway Safety Equipment Technician
Office of Public Safety

**SIMULATOR
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Geddes Town Police Department
Manufacturer: GUTH LABORATORIES
Model: 12V500
Serial Number: MP4203
Date: May 25, 2021

1. General appearance and condition of this device -----: OK

2. Check propeller rotation -----: OK

3. Check for air leaks -----: OK

4. Check for proper temperature -----:OK

**5. Record any repairs made to this instrument and list services provided: VERIFIED
CALIBRATION**



Martin Schilling
Highway Safety Equipment Technician
Office of Public Safety

NIST Traceable
Calibration Report



Reference Number: 1401243
 PO Number: MCANARY031121

New York State Division Criminal Justice Services
 80 South Swan Street
 Albany NY 12210

Manufacturer: Alpha Technics
Model Number: 91-5443
Description: Temperature, Thermometer
Asset Number: 20BMM01712
Serial Number: 20BMM01712
Procedure: DS Alpha Technics 5000 Series f/NY State DCJS

Calibration Date: 03/16/2021
Calibration Due Date: 03/16/2022
Condition As Found: In Tolerance
Condition As Left: In Tolerance, No adjustment

Remarks:
 NIST-traceable calibration performed on the unit referenced above in accordance with customer requirements, published specifications and the lab's standard operating procedures. No adjustments were made to the unit.

Standards Utilized

Asset No.	Manufacturer	Model No.	Description	Cal. Date	Due Date
CP144317	Fluke Corporation	1595A	Thermometer, Readout, Precision Thermometer	01/28/2020	02/28/2022
CP32033	Hart Scientific	5628	Temperature, Probe	10/08/2019	04/30/2021
CP32034	Hart Scientific	5628	Temperature, Probe	01/22/2020	10/31/2021
CP50205	Hart Scientific	5628	Temperature, Probe	03/12/2020	02/28/2022
CP53595	Hart Scientific	5628	Temperature, Probe	01/28/2020	02/28/2022

Calibration Data

FUNCTION TESTED	Nominal Value	As Found	Out of Tol	As Left	Out of Tol	CALIBRATION TOLERANCE
Temperature	-15.000 °C	-14.99		Same		-15.050 to -14.950 °C [EMU 0.0099 °C][TUR 5.1:1]
	0.000 °C	0.01		Same		-0.030 to 0.030 °C [EMU 0.0072 °C][TUR 4.2:1]
	75.000 °C	75.00		Same		74.970 to 75.030 °C [EMU 0.011 °C][TUR 2.7:1]
	125.000 °C	124.99		Same		124.950 to 125.050 °C [EMU 0.011 °C][TUR 4.5:1]

Temperature: 22° C
Humidity: 36% RH
Rpt. No.: 1645707

Calibration Performed By:			Quality Reviewer:	
Sittinger, Jennifer	Metrologist	847-327-5317	Szplit, Tony	03/17/2021
Name	Title	Phone	Name	Date

This report may not be reproduced, except in full, without written permission of Innocal. The results stated in this report relate only to the items tested or calibrated. Measurements reported herein are traceable to SI units via national standards maintained by NIST and were performed in compliance with MIL-STD-45682A, ANSI/NCSL Z540-1-1994, 10CFR50, Appendix B, ISO 9002-94, and ISO 17025:2017. Guard Banding, if reported on this certificate, is applied at a Z-factor of 30% for test points with a test uncertainty ratio (TUR) below 4:1. The estimated measurement uncertainty (EMU), if reported on this certificate, is being reported at a confidence level of 95% or K=2 unless otherwise noted in the remarks section.

